





APPROVED

PRINT NAME:
DATE:
SIGNATURE:

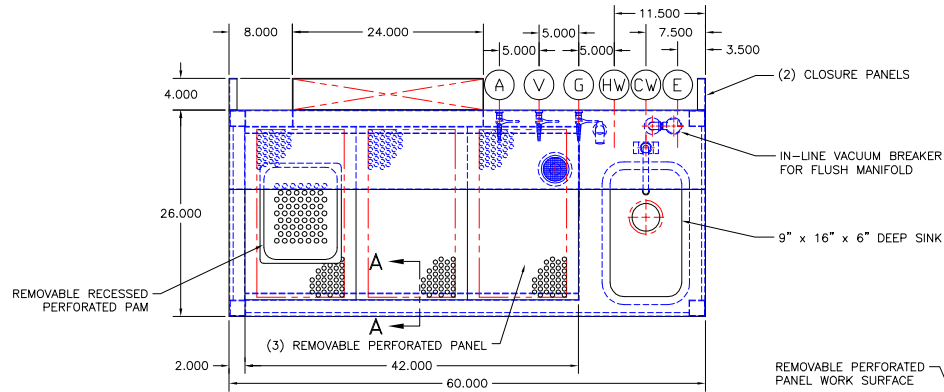


- UTILITY REQUIREMENTS
- (E) — ELECTRICAL - 115 V., 1 PH., 60 Hz., 20 AMP.
 - (CW) — COLD WATER - 3/4" I.P.S.
 - (HW) — HOT WATER - 1/2" I.P.S.
 - (D) — DRAIN - 1-1/2" NPT FLOOR DRAIN MIN.
 - (EX) — EXHAUST - 4" x 24" OUTSIDE DIM.

- INCLUDED OPTIONS
- REMOVABLE PERFORATED PAN
 - AUTOMATIC HEIGHT ADJUSTMENT
 - 1 HP HEAVY DUTY DISPOSER
 - MANUALLY ADJUSTABLE DUCT DAMPER
 - REMOVABLE HOOD WITH HINGED VIEWING WINDOW
 - MAGNETIC INSTRUMENT BAR
 - ADJUSTABLE ARM SWIVEL TYPE SURGICAL LAMP
 - VACUUM OUTLET
 - GAS OUTLET
 - AIR OUTLET

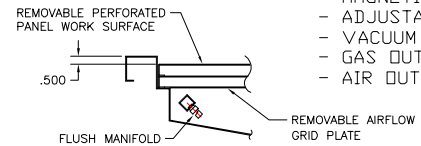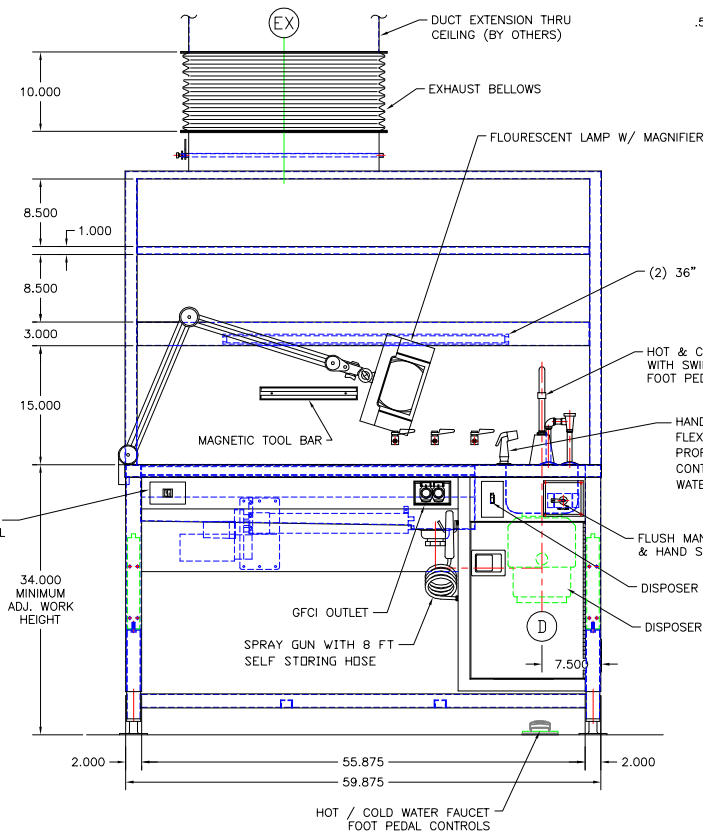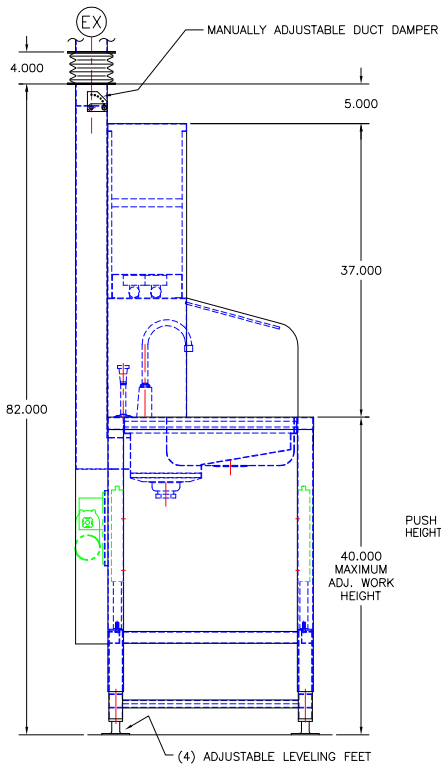

SECTION A-A

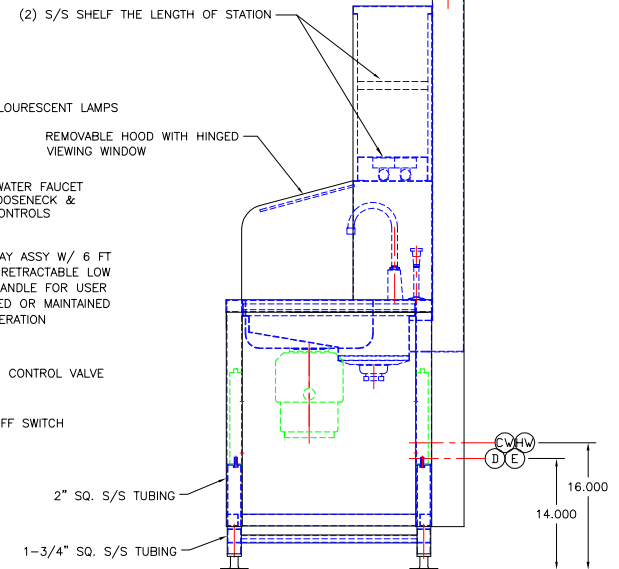

NOTE: T316 STAINLESS STEEL CONSTRUCTION

This print is the property of TBJ Incorporated. The information contained herein is confidential, it is not transferable. It is furnished with the clear understanding that it is not to be traced, reproduced or used in any other process of manufacturing without written permission from the owner and is returnable upon request.

TBJ INC				1671 ORCHARD DRIVE CHAMBERSBURG, PA 17201	
SCALE 1-1/2"=1'-0"		DRAWN BY CWF		DATE 10-10-05	
REF DWG - R03058		MODEL 26-60 3D		DDWDRAFT NECROPSY/TRIM STATION	
LET	REVISION	BY	DATE	ROUGH-IN ASSEMBLY	R05190