


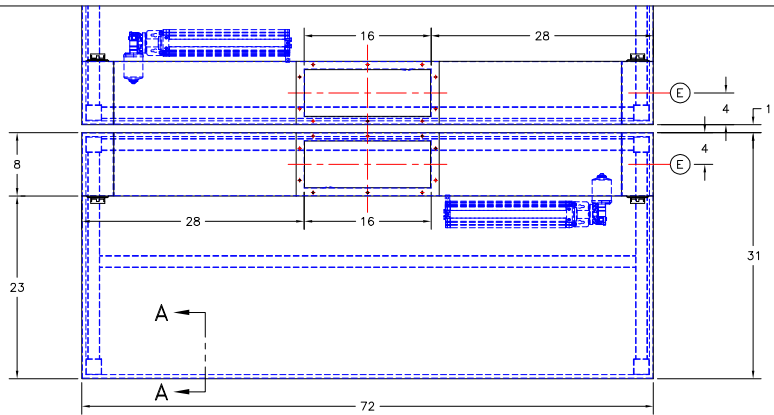

UTILITY REQUIREMENTS




- (E) — ELECTRICAL - (2) @ 115 V., 1 PH., 60 Hz., 15 AMP
 (EX) — EXHAUST - (2) @ 16" X 6" OUTSIDE DIMS., 475 CFM @ 0.25 S.P.

APPROVED

PRINT NAME:


DATE:

SIGNATURE:

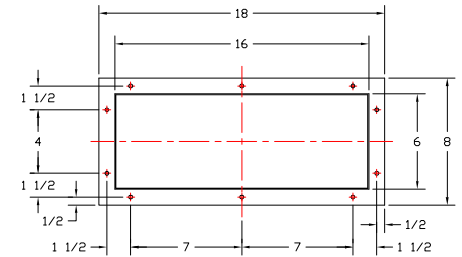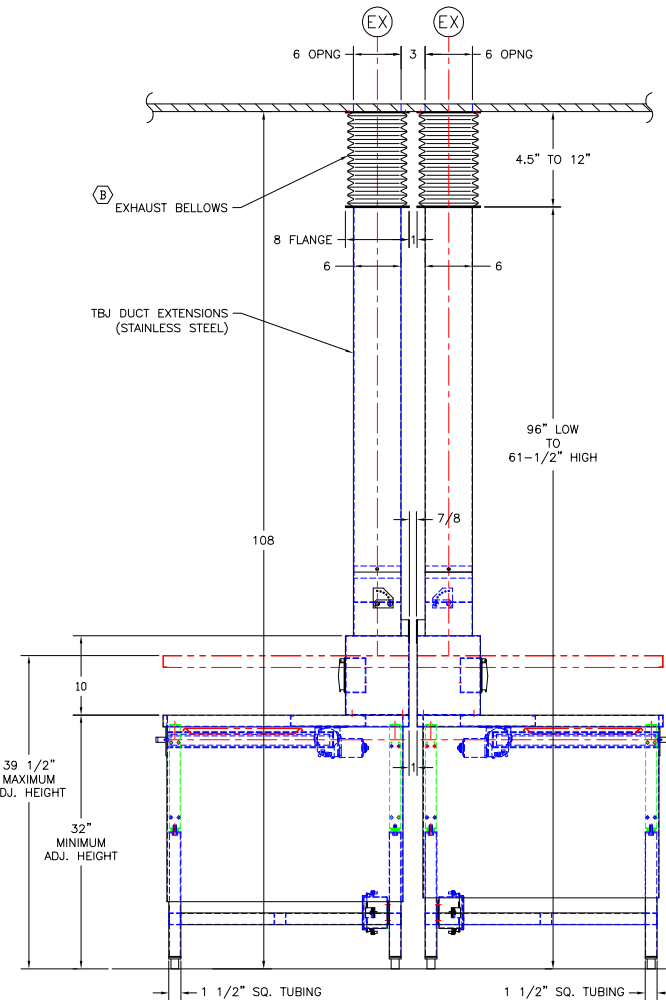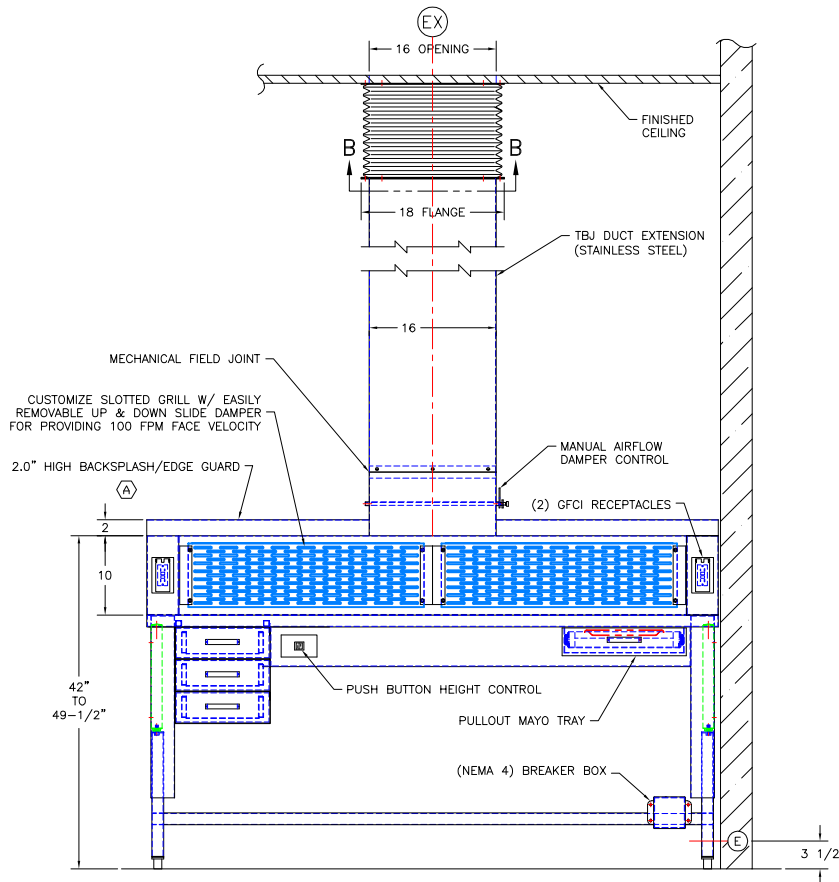

SECTION B-B

SCALE: 3"=1'-0"

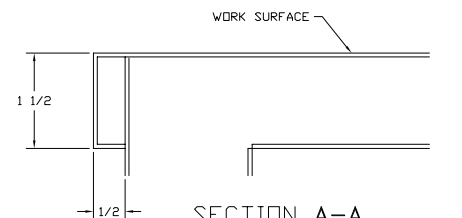

SECTION A-A

SCALE: FULL

V-8

NECROPSY ROOM

B	MOVED BELLOW TRANSITION TO FINISHED CEILING	ALE	12-15-09
A	ADDED EDGE GUARD & A SECOND GFCI	ALE	8-17-09
LET	REVISION	BY	DATE
		1671 ORCHARD DRIVE CHAMBERSBURG, PA 17201	
SCALE: 1-1/2"=1'-0"		DRAWN BY: ALE	
REF DWG - R07121		DATE: 8-14-09	
MODEL 31-60 BD			
BACKDRAFT SURGERY TABLE			
ROUGH-IN ASSEMBLY			R09140